

This article was downloaded by:[Nieman, David C.]
[Nieman, David C.]

On: 26 March 2007

Access Details: [subscription number 772610559]

Publisher: Taylor & Francis

Informa Ltd Registered in England and Wales Registered Number: 1072954

Registered office: Mortimer House, 37-41 Mortimer Street, London W1T 3JH, UK



Research in Sports Medicine An International Journal

Publication details, including instructions for authors and subscription information:
<http://www.informaworld.com/smpp/title-content=t713926139>

Validation of Cosmed's FitMate™ in Measuring Exercise Metabolism

To cite this Article: , 'Validation of Cosmed's FitMate™ in Measuring Exercise Metabolism', Research in Sports Medicine, 15:1, 67 - 75

xxxx:journal To link to this article: DOI: 10.1080/15438620601184380

URL: <http://dx.doi.org/10.1080/15438620601184380>

Full terms and conditions of use: <http://www.informaworld.com/terms-and-conditions-of-access.pdf>

This article maybe used for research, teaching and private study purposes. Any substantial or systematic reproduction, re-distribution, re-selling, loan or sub-licensing, systematic supply or distribution in any form to anyone is expressly forbidden.

The publisher does not give any warranty express or implied or make any representation that the contents will be complete or accurate or up to date. The accuracy of any instructions, formulae and drug doses should be independently verified with primary sources. The publisher shall not be liable for any loss, actions, claims, proceedings, demand or costs or damages whatsoever or howsoever caused arising directly or indirectly in connection with or arising out of the use of this material.

© Taylor and Francis 2007

VALIDATION OF COSMED'S FitMate™ IN MEASURING EXERCISE METABOLISM

David C. Nieman
Heather LaSasso
Melanie D. Austin
Steven Pearce
Tim McInnis
Jess Unick

Department of Health, Leisure, and Exercise Science, Human Performance
Lab, Appalachian State University, Boone, North Carolina, USA

The purpose of this study was to assess the validity of the FitMate™ metabolic system (Cosmed, Rome, Italy) in measuring oxygen consumption during graded exercise. The FitMate™ is a new, small (20 × 24 cm) metabolic analyzer designed for measurement of oxygen consumption during rest and exercise. Subjects included 40 healthy adults (N = 20 males, N = 20 females) ranging in age from 18 to 37 kg/m² (mean ± SD age, 22.5 ± 3.6 years) and body mass index (BMI) from 18.3 to 32.5 kg/m² (23.2 ± 3.3 years). One-minute FitMate™ and Douglas bag measurements were made during steady state conditions at the end of each 3-minute stage of the Bruce treadmill graded exercise test, and subjects continued until they could not attain steady state exercise during a stage. Oxygen consumption difference scores (Douglas bag minus FitMate™ measurements) did not differ between males and females, so data were combined and analyzed for the entire group. During the first three stages, mean oxygen consumption did not differ significantly between the Douglas bag and FitMate™ systems (26.5 ± 1.1 and 26.7 ± 1.3 ml·kg⁻¹·min⁻¹, respectively, P = 0.140) with a mean absolute difference of 0.23 ± 0.91 ml·kg⁻¹·min⁻¹ or 14.2 ± 67.5 ml·min⁻¹. In conclusion, the FitMate™ metabolic system accurately measures oxygen consumption during graded treadmill exercise when compared with the Douglas bag system in male and female adults.

Received 5 June 2006; accepted 5 December 2006.

This research was funded in part by Cosmed (Rome, Italy).

Address correspondence to David C. Nieman, Department of Health, Leisure, and Exercise Science, Appalachian State University, P.O. Box 32071, 111 Rivers Street, Holmes Convocation Center, Boone, NC 28608, USA. E-mail: niemandc@appstate.edu

INTRODUCTION

One of the most common measurements made by exercise science professionals is oxygen consumption during both rest and exercise. Oxygen consumption during exercise can be measured using human calorimeters, closed-circuit indirect calorimetry equipment, and open-circuit indirect calorimetry equipment such as Douglas bags, gas analyzers, whole body respiratory chambers, and computerized metabolic carts (Macfarlane 2001; Meyer, Davison, and Kindermann 2005). These methods are costly, cumbersome to conduct, and require highly skilled technicians, making them impractical for most clinical and community settings. Studies show that automated metabolic systems often vary when compared with one another or with the Douglas bag system (Carter and Jeukendrup 2002; Rietjens et al. 2001; Foss and Hallen 2005; Miles, Cox, and Verde 1994; Gore et al. 2003; Bassett et al. 2001).

During the past 40 years, various portable metabolic devices have been developed to facilitate oxygen consumption measurements in nonlaboratory settings. Validation studies have been published for several of these devices, including the K4b2 from Cosmed (Duffield, Dawson, and Pinnington 2004; Eisenmann et al. 2003; McLaughlin et al. 2001; McNaughton et al. 2005; Pinnington et al. 2001), K2 from Cosmed (Crandall, Taylor, and Raven 1993; Lucia et al. 1993), VO2000 from Medical Graphics (Crouter et al. 2006; Wahrlich et al. 2006) and its predecessor Aerosport TEEM 100 and KB1-C from Aerosport Inc. (King et al. 1999), VmaxST from Sensor Medics (Brehm, Harlaar, and Groepenhof 2004), and MetaMax II from CORTEX Biophysik (Larsson et al. 2004). Although these portable metabolic devices are accurate, they still pose problems when considering cost and ease of use.

A small, hand-held, and easy-to-use metabolic system, the BodyGem/MedGem (HealtheTech, Golden, CO), was developed for accurate measurement of resting oxygen consumption and energy expenditure (Nieman, Trone, and Austin 2003; Nieman et al. 2005; Stewart, Goody, and Branson, 2005; St-Onge et al. 2004). The BodyGem/MedGem, however, was not designed for measurement of oxygen consumption during exercise. The FitMate™ from Cosmed Inc. (Rome, Italy) is a small, easy-to-use, inexpensive, and accurate metabolic analyzer that is designed for metabolic measurements during graded exercise. Previously, we validated the use of the FitMate™ in measuring resting oxygen consumption and energy expenditure (Nieman et al. 2006). The FitMate™ utilizes new sampling technology through the use of a representative small sample of the expired volume in a miniaturized dynamic mixing chamber. The FitMate™ uses a turbine flowmeter for measuring ventilation and a galvanic fuel cell oxygen sensor for analyzing fraction of expired oxygen.

The FitMate™ does not have a CO₂ analyzer and relies on a software paradigm that ramps the respiratory exchange ratio (RER) between 0.8 and 1.2 based on the increase in heart rate.

Validation studies have not yet been conducted to test whether the unique features of the FitMate™ allow for accurate measurement of oxygen consumption during graded exercise. Therefore, the purpose of this study was to assess the validity of the FitMate™ metabolic system when compared with the Douglas bag system in measuring oxygen consumption and ventilation in male and female adults during graded exercise on a treadmill.

METHODS

Subjects

Subjects included 20 men and 20 women between the ages of 18 and 37 years. Subjects came to the Appalachian State University (ASU) Human Performance Lab between 3:30 and 5:30 p.m. for one test session. Prior to the treadmill test, a screening questionnaire was used to determine health and disease status, followed by measurement of height and weight, and an orientation to the testing procedures. Testing procedures were approved by the university's internal review board prior to initiation of the study. Subjects voluntarily gave informed consent.

Research Design

The Bruce treadmill graded exercise test was used with 1-minute measurements made by the Cosmed FitMate™ and the Douglas bag systems during steady state after exercising for 3 minutes during each treadmill stage. Prior to starting the treadmill test, subjects were fitted with a face-mask that was used for all metabolic measurements. After exercising for 3 minutes in a treadmill stage, 1-minute measurements were first made with the FitMate™ followed by removal of the FitMate™ turbine flow meter and sampling line, and then attachment to the face mask of a two-way Hans-Rudolph valve (Hans-Rudolph Inc., Kansas City, MO) and hose for a 1 minute collection of expired air in a Douglas bag. The first stage of the Bruce treadmill test was set at 1.7 mph and 10% grade (easy), the second stage at 2.5 mph and 12% grade (light exertion), the third stage at 3.4 mph and 14% grade (brisk uphill walk, moderate exertion for most), the fourth stage at 4.0 mph and 16% grade (uphill jog, hard exertion for most), and the fifth stage at 4.5 mph and 18% grade. Subjects continued until they could attain steady state exercise (or the ability to hold the pace without tiring) during a stage.

Douglas Bag Testing Procedures

Douglas bag collections of expired gases were made for 1 minute using a facemask connected to a Hans-Rudolph two-way valve (Hans-Rudolph Inc., Kansas City, MO). Expired gas fractions were analyzed using an Applied Electrochemistry S-3A oxygen analyzer and an Applied Electrochemistry CD-3A carbon dioxide analyzer (AEI Technologies, Applied Electrochemistry, Pittsburgh, PA). The analyzers were calibrated using a two-point method with outside air and medical grade primary standard gases containing 16.0% O₂ and 4.0% CO₂ (Matheson Tri-Gas, Parsippany, NJ). Expired gas volumes were measured using a Rayfield RAM 9200 air flowmeter (Waitsfield, VT) calibrated against a Tissot spirometer.

FitMate™ Testing

The FitMate™ is a new, small (20 × 24 cm) metabolic analyzer designed for the measurement of oxygen consumption and energy expenditure during rest and exercise (Cosmed, Rome, Italy). It uses a turbine flowmeter for measuring ventilation and a galvanic fuel cell oxygen sensor for analyzing the fraction of expired oxygen, and it incorporates a patented sampling technology that allows FitMate™ performance to be comparable with the performance of a metabolic cart with a standard mixing chamber. The FitMate™ uses a representative small sample of expired volume in a dynamic mixing chamber to analyze fractions of expired oxygen (FeO₂). The FitMate™ system has an automatic recalibration system using room air, recalibrating periodically during the test without any interruptions. This is possible because there is no CO₂ analyzer, and the O₂ sensor is intrinsically linear (a single-point calibration ensures accuracy in the entire range of measurements). Without CO₂ data, VO₂ is calculated intrinsically with the use of the equation $VO_2 = (FiO_2 \cdot IV - FeO_2 \cdot EV) \cdot RF \cdot STPD$, where RF = respiratory frequency, IV = inspired volume, EV = expired volume, FiO₂ = fraction of inspired O₂, and FeO₂ = fraction of expired O₂. Inspired volume is calculated using the Haldane correction, $IV = (100 + R \cdot (FeO_2 - 20.93) - FeO_2) \cdot EV / 79.04$, where R = respiratory exchange ratio. R is estimated by ramping values linearly between 0.8 and 1.2 in accordance with the increase in heart rate during exercise. Sensors measure temperature and barometric pressure for use in internal calculations.

Statistical Analysis

FitMate™ and Douglas bag oxygen consumption and metabolic measurements were compared using paired *t* tests with difference scores computed

between methods (Douglas bag – FitMate™). Statistical significance was set at the $p \leq 0.05$ level, and values were expressed as mean \pm SD.

RESULTS

Forty subjects (20 males and 20 females) completed all phases of the study. Subject characteristics are reported in Table 1, with data summarized for age, stature, body mass, and BMI (kg/m^2). For all subjects combined, age ranged from 18 to 37 years, and BMI from 18.3 to 32.5 kg/m^2 .

No difference was found between males and females for the primary outcome measures, and the data are presented for all subjects combined (Table 2 and Figure 1). When combining data from treadmill stages 1, 2, and 3 ($N = 35$ subjects), no significant differences were found between Douglas bag and FitMate™ systems for oxygen consumption (26.5 ± 1.1 and $26.7 \pm 1.2 \text{ ml}\cdot\text{kg}^{-1}\cdot\text{min}^{-1}$, respectively, $P = 0.140$), with a mean difference of $0.23 \pm 0.91 \text{ ml}\cdot\text{kg}^{-1}\cdot\text{min}^{-1}$ (or $14.2 \pm 67.5 \text{ ml}\cdot\text{min}^{-1}$). Only 10 subjects completed stage 4, and oxygen consumption was slightly but significantly higher during the Douglas bag measurement, in part due to an “order effect” (see next paragraph). Figure 1 depicts scatterplot data comparing FitMate™ and Douglas bag systems during each stage of the Bruce treadmill test. The line of best fit for the entire data set was nearly identical in slope to the line of identity (dashed line).

Due to methodological issues, measurements at the end of each 3-minute treadmill stage were taken first with the FitMate™ system followed by the Douglas bag system, a process that took about 3 minutes. This measurement order effect resulted in small but significant differences in FeO_2 , ventilation, and heart rate between the FitMate™ and Douglas bag systems (Table 2).

Table 2 summarizes FeCO_2 and RER data from the Douglas bag measurements, and respiratory rate data from the FitMate™ system. Comparisons between systems were not possible because the FitMate™ system does not have a CO_2 analyzer, and the Douglas bag system does not provide respiratory rate measurements.

Table 1. Subject Characteristics for Male ($n = 20$) and Female ($n = 20$) Subjects (mean \pm SD)

| Variable | Males | Females |
|--|-----------------|-----------------|
| Age (yrs) | 23.5 ± 4.1 | 21.5 ± 2.8 |
| Stature (m) | 1.79 ± 0.05 | 1.63 ± 0.07 |
| Body mass (kg) | 79.7 ± 12.9 | 57.8 ± 7.4 |
| Body mass index (kg/m^2) | 24.9 ± 3.4 | 21.6 ± 2.4 |

Table 2. Comparison of Oxygen Consumption (VO₂), Ventilation, and Other Metabolic Values Between the FitMate and Douglas Bag Methods During Steady State Exercise for the First Three Stages of the Bruce Treadmill Test (mean ± SD)

| | Stage 1 (N = 40) | Stage 2 (N = 40) | Stage 3 (N = 35) | Stage 4 (N = 10) |
|---|---------------------|---------------------|---------------------|---------------------|
| VO ₂ (ml·kg ⁻¹ ·min ⁻¹) | | | | |
| Douglas bag | 17.3 ± 1.0 | 25.4 ± 1.3 | 36.8 ± 1.9 | 52.4 ± 2.3 |
| FitMate | 17.8 ± 1.2** | 25.7 ± 1.6 | 36.7 ± 2.0 | 50.7 ± 2.8** |
| FeO ₂ (%) | | | | |
| Douglas bag | 15.9 ± 0.5 | 15.8 ± 0.6 | 16.2 ± 0.7 | 16.4 ± 0.5 |
| FitMate | 15.2 ± 0.5** | 15.4 ± 0.5** | 15.8 ± 0.6** | 16.0 ± 0.4** |
| Ventilation (l·min ⁻¹) | | | | |
| Douglas bag | 30.7 ± 7.1 | 45.0 ± 10.2 | 70.4 ± 14.5 | 117 ± 20 |
| FitMate | 28.6 ± 6.0** | 43.6 ± 10.1 | 67.5 ± 14.1** | 105 ± 13** |
| Heart rate (beats·min ⁻¹) | | | | |
| Douglas bag | 110 ± 15 | 137 ± 20 | 168 ± 21 | 181 ± 12 |
| FitMate | 105 ± 14** | 132 ± 21** | 162 ± 21** | 177 ± 12** |
| FeCO ₂ (%) | | | | |
| Douglas bag | 4.32 ± 0.45 | 4.69 ± 0.51 | 4.69 ± 0.59 | 4.64 ± 0.51 |
| RER | | | | |
| Douglas bag | 0.81 ± 0.05 | 0.88 ± 0.05 | 0.97 ± 0.06 | 1.03 ± 0.06 |
| RR (breaths·min ⁻¹) | | | | |
| FitMate | 22.9 ± 4.7 | 27.6 ± 5.3 | 34.3 ± 7.3 | 39.6 ± 6.3 |

VO₂ = volume of oxygen consumed; FeO₂ = fraction of expired oxygen; FeCO₂ = fraction of expired carbon dioxide; RER = respiratory exchange ratio; RR = respiratory rate.

*P value < 0.05; **P value < 0.01 when comparing FitMate and Douglas bag systems.

DISCUSSION

The purpose of this study was to compare the Douglas bag system with the FitMate™, a small, portable metabolic device used to measure oxygen consumption during both rest and exercise. The data from a group of 40 young male and female adults indicated that the FitMate™ gave accurate oxygen consumption measurements when compared with the Douglas bag method. When measurements from the first three stages of the Bruce treadmill protocol were averaged and compared, the mean difference for oxygen consumption was small and statistically insignificant. This indicates that graded exercise testing with the FitMate™ will give accurate oxygen consumption measurements.

Other small metabolic devices have been developed for measuring oxygen consumption and ventilation, but they are expensive and require skilled technicians. The FitMate™ is easy to use, inexpensive, and small,

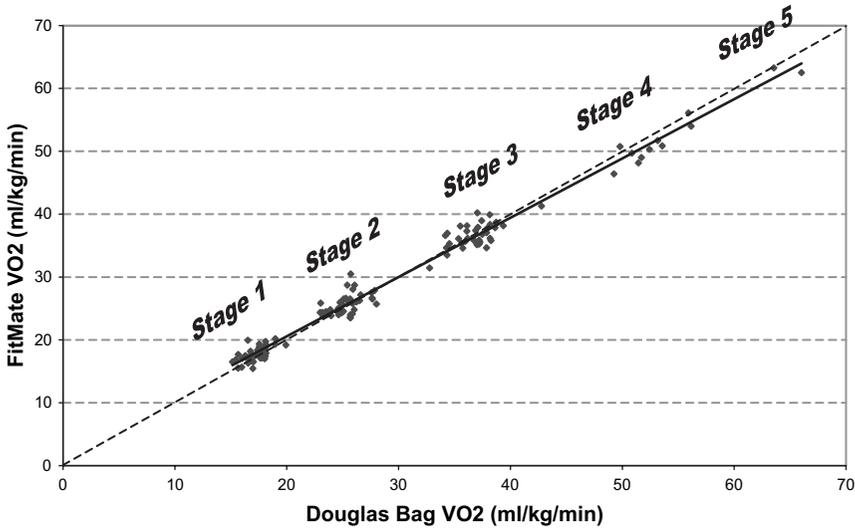


Figure 1. Scatterplot VO2 Douglas bag versus FitMate.

but it does not have a CO₂ analyzer. Our data indicate that ramping the RER between 0.8 and 1.2 in accordance with the increase in heart rate results in minimal error. For example, during the second treadmill stage, RER varied between 0.81 and 1.095 as measured with the Douglas bag system, with a group mean of 0.88. This range in RER would cause a variation in VO₂ estimates of about 7.5%, but this error was markedly reduced with the Cosmed ramping paradigm.

The K2 from Cosmed Inc. (Rome, Italy) was another portable metabolic system that lacked a CO₂ analyzer (Crandall et al. 1993; Lucia et al. 1993). Since there was no CO₂ analyzer, the K2 assumed a constant RER of 1.0 for all exercise workloads. In one study, the K2 underestimated VO₂ at lower workloads and overestimated VO₂ at higher workloads due to the assumption of a constant RER of 1.0 (Crandall et al. 1993). Studies indicated that when the subjects' actual RER value was measured with the Douglas bag system or other metabolic systems, and the K2 calculations were corrected using the true RER value, errors in VO₂ estimates during graded exercise were diminished (Crandall et al., 1993; Lucia et al. 1993). Since the FitMate™ increases RER in a linear relationship to heart rate during maximal graded exercise from 0.8 to 1.2, this calculation eliminates the type of error that occurred with the K2 by assuming an RER of 1.0.

The FitMate™ system utilizes a facemask with a turbine device and a sampling line, thus prohibiting simultaneous measurement of oxygen

consumption and ventilation with the Douglas bag system. Due to the intrinsic workings of the FitMate™ metabolic system, the FitMate™ measurements had to be made prior to the Douglas bag measurements during each stage. This resulted in small but significant differences in FeO_2 , ventilation, and heart rate between the FitMate™ and Douglas bag systems. These differences, however, were more than likely due to a small drift in metabolic responses during 2 to 3 minutes of measurements during steady state exercise at the end of each 3-minute treadmill stage.

In conclusion, the FitMate™ metabolic system accurately measured oxygen consumption during graded treadmill exercise in male and female young adults. Despite the lack of a CO_2 analyzer, the system adequately adjusted by ramping RER in accordance with the heart rate. The dynamic, miniaturized mixing chamber with intrinsic adjustments for RER allowed for accurate measurements of oxygen consumption by the FitMate™ system. Another unique feature of the FitMate™ is that calibration occurs automatically just prior to exercise and at set intervals during the exercise test without interruption. The FitMate™ is a small, inexpensive, user-friendly, lightweight, battery-powered unit, facilitating accurate metabolic measurements in both the field and in the lab.

REFERENCES

- Bassett DR, Howley ET, Thompson DL, King GA, Strath SJ, McLaughlin JE, Parr BB (2001) Validity of inspiratory and expiratory methods of measuring gas exchange with a computerized system. *Journal of Applied Physiology* 91: 218–224.
- Brehm MA, Harlaar J, Groepenhof H (2004) Validation of the portable VmaxST system for oxygen uptake measurement. *Gait and Posture* 20: 67–73.
- Carter J, Jeukendrup AE (2002) Validity and reliability of three commercially available breath-by-breath respiratory systems. *European Journal of Applied Physiology* 86: 435–441.
- Crandall CG, Taylor SL, Raven PB (1993) Evaluation of the Cosmed K2 portable telemetric oxygen uptake analyzer. *Medicine and Science in Sports and Exercise* 26: 108–111.
- Crouter SE, Antczak A, Hudak JR, DellaValle DM, Haas JD (2006) Accuracy and reliability of the ParvoMedics TrueOne 2400 and MedGraphics VO2000 metabolic systems. *European Journal of Applied Physiology* 98: 139–151.
- Duffield R, Dawson B, Pinnington HC, Wong P (2004) Accuracy and reliability of a Cosmed K4b² portable gas analysis system. *Journal of Science and Medicine in Sport* 7(1): 11–22.
- Eisenmann JC, Brisko N, Shadrick D, Welsh S (2003) Comparative analysis of the Cosmed Quark b² and K4b² gas analysis systems during submaximal exercise. *Journal of Sports Medicine and Physical Fitness* 43: 150–155.
- Foss O, Hallen J (2005). Validity and stability of a computerized metabolic system with mixing chamber. *International Journal of Sports Medicine* 26: 569–575.

- Gore CJ, Clark RJ, Shipp NJ, VanDerPloeg GE, Withers RT (2003) CPX/D underestimates VO_2 in athletes compared with an automated Douglas bag system. *Medicine and Science in Sports and Exercise* 35: 1341–1347.
- King GA, McLaughlin JE, Howley ET, Basset DR, Ainsworth BE (1999) Validation of Aerosport KB1-C portable metabolic system. *International Journal of Sports Medicine* 20: 304–308.
- Larsson PU, Wadell KME, Jakobsson EJI, Burlin LU, Henriksson-Larsén KB (2004) Validation of the MetaMax II portable metabolic measurement system. *International Journal of Sports Medicine* 25: 115–123.
- Lucia A, Fleck SJ, Gotshall RW, Kearney JT (1993) Validation and reliability of the Cosmed K2 instrument. *International Journal of Sports Medicine* 14: 380–386.
- Macfarlane DJ (2001) Automated gas analysis systems: A review. *Sports Medicine* 31(12): 841–861.
- McLaughlin JE, King GA, Howley ET, Basset DR, Ainsworth BE (2001) Validation of the Cosmed K4b² portable metabolic system. *International Journal of Sports Medicine* 22: 280–284.
- McNaughton LR, Sherman R, Roberts S, Bentley DJ (2005) Portable gas analyzer Cosmed K4b² compared to a laboratory based mass spectrometer system. *Journal of Sports Medicine and Physical Fitness* 45: 315–323.
- Meyer T, Davison RCR, Kindermann W (2005) Ambulatory gas exchange measurements—Current status and future options. *International Journal of Sports Medicine* 26(Suppl 1): S19–S27.
- Miles DS, Cox MH, Verde TJ (1994) Four commonly utilized metabolic systems fail to produce similar results during submaximal and maximal exercise. *Sports Medicine Training and Rehabilitation* 5: 189–198.
- Nieman DC, Austin MD, Benezra L, Pearce S, McInnis T, Gross SJ (2006) Validation of Cosmed's FitMate™ in measuring oxygen consumption and estimating resting metabolic rate. *Research in Sports Medicine* 14: 89–96.
- Nieman DC, Austin MD, Chilcote SM, Benezra L (2005) Validation of a new handheld device for measuring resting metabolic rate and oxygen consumption in children. *International Journal of Sport Nutrition, Exercise, and Metabolism* 14: 208–216.
- Nieman DC, Trone GA, Austin MD (2003) A new handheld device for measuring resting metabolic rate and oxygen consumption. *Journal of the American Dietetic Association* 103(5): 587–593.
- Pinnington HC, Wong P, Tay J, Green D, Dawson B (2001) The level of accuracy and agreement in measures of F_EO_2 , F_ECO_2 and V_E between the Cosmed K4b² portable, respiratory gas analysis system and a metabolic cart. *Journal of Science and Medicine in Sport* 4(3): 324–335.
- Rietjens GJWM, Kuipers H, Kester ADM, Keizer HA (2001) Validation of a computerized metabolic measurement system (Oxycon-Pro®) during low and high intensity exercise. *International Journal of Sports Medicine* 22: 291–294.
- Stewart CL, Goody CM, Branson R (2005) Comparison of two systems of measuring energy expenditure. *Journal of Parenteral and Enteral Nutrition* 29(3): 212–217.
- St-Onge MP, Rubiano F, Jones A, Heymsfield SB (2004) A new hand-held indirect calorimeter to measure postprandial energy expenditure. *Obesity Research* 12: 704–709.
- Währlich V, Anjos LA, Going SB, Lohman TG (2006) Validation of the VO2000 calorimeter for measuring resting metabolic rate. *Clinical Nutrition* 25: 687–692.